FRESENIUS MEDICAL CARE

Liberty® Select Cycler Drain Logic
Support Guide

The purpose of this guide is to illustrate how the Liberty Select cycler determines the next appropriate step after detecting a **low drain rate of <30mL/min**.

Volume Check
Has at least 70% or 85% of the previous fill volume drained?

Proceed to Next Fill
End drain phase and proceed to next fill phase.

Overfill Check
Is the **Expected drain** minus the **Actual drain**, plus the **Next fill**, greater than **150%** of the **Prescribed fill volume**?

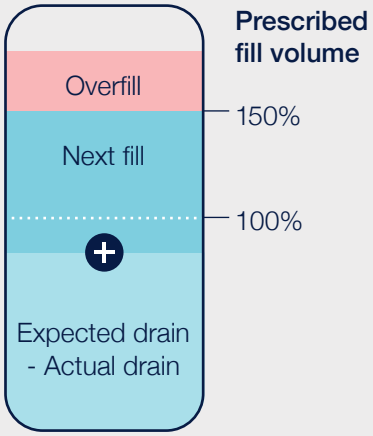

Drain 0

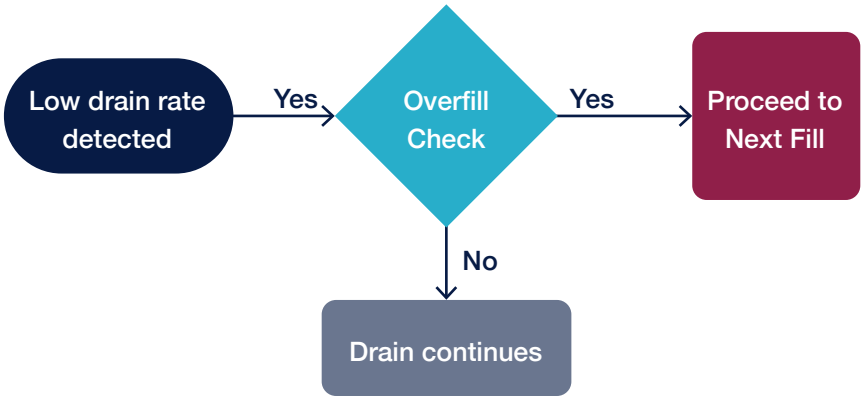

All other drains

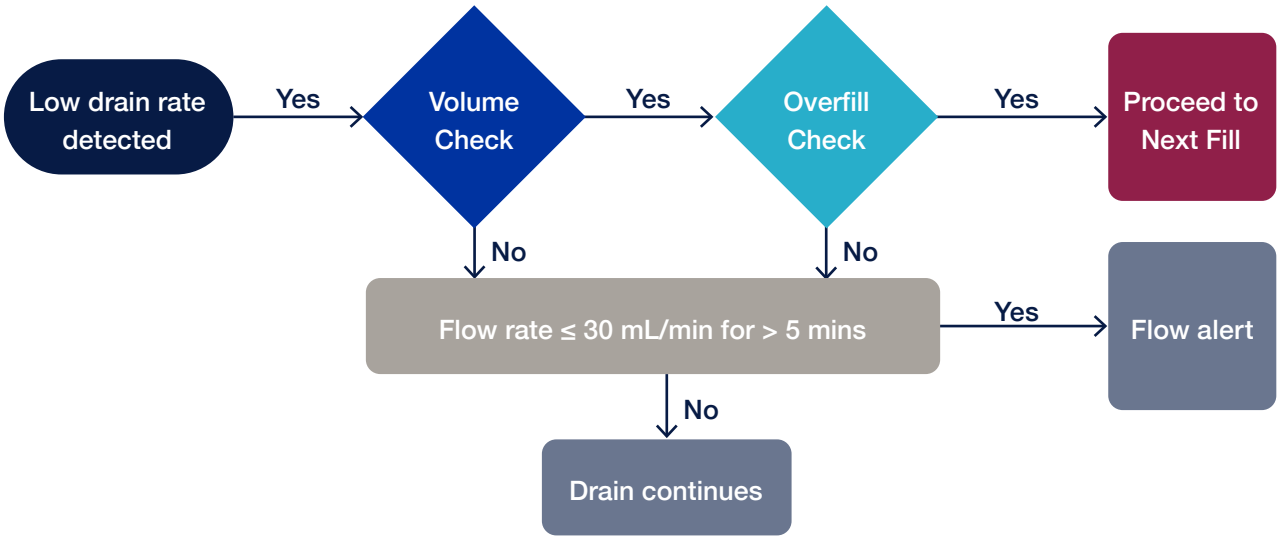

Read the Instructions for Use for safe and proper use of this device. For a complete description of hazards, contraindications, side effects, and precautions, see full package labeling at www.fmcna.com

Indications for Use: The Fresenius Liberty Select Cycler is indicated for acute and chronic peritoneal dialysis.

Caution: Federal (US) law restricts this device to sale by or on the order of a physician.

© 2026 Fresenius Medical Care. All Rights Reserved. Fresenius Medical Care, the triangle logo, and Liberty are trademarks for which Fresenius Medical Care AG holds rights. All other trademarks are the property of their respective owners. P/N 105784-01 Rev A 09/2026