FRESENIUS MEDICAL CARE

Liberty® Select Cycler Time/Date Change
Quick Help Guide

Treatment data may not transmit to your dialysis center if this information is incorrect.

Note that you cannot change the date or time during set up or while in treatment.

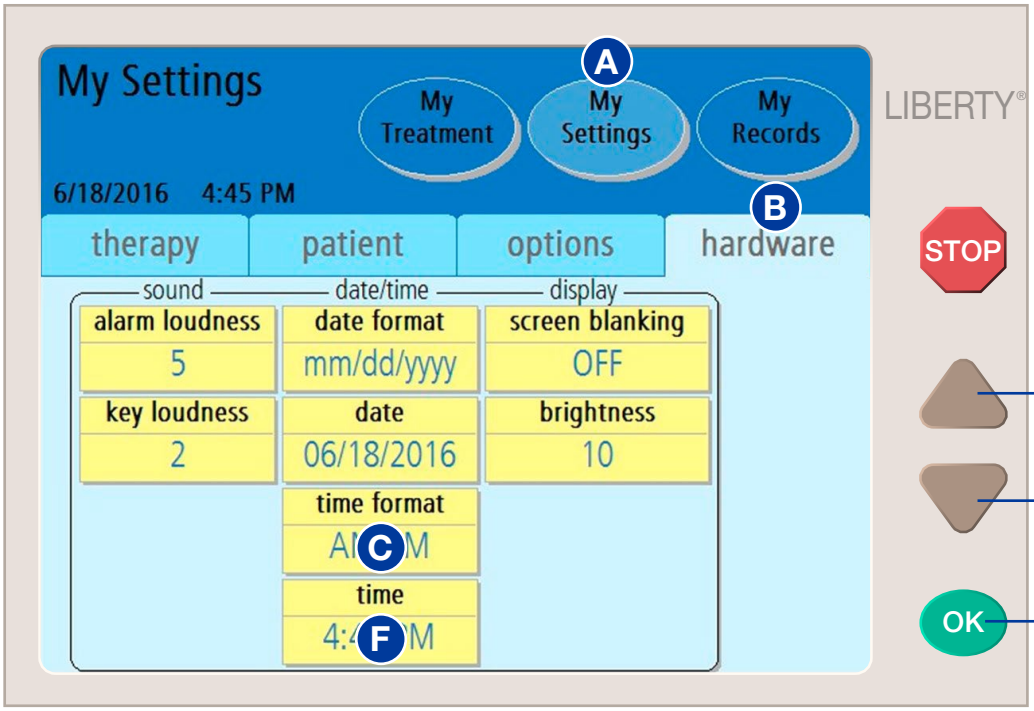

Changing the time

1. Select **My Settings**	A	**6.** Select **time** (Button turns orange)	F
2. Select **hardware** tab	B	**7.** Use the arrow keys to select the **hour**	D
3. Select **time format** (Button turns orange)	C	**8.** Select **OK** to save and proceed to *minute*	E
4. Use the arrow keys to select **AM/PM**	D	**9.** Use the arrow keys to select the **minute**	D
5. Select **OK** to save (Button turns yellow)	E	**10.** Select **OK** to save (Button turns yellow)	E

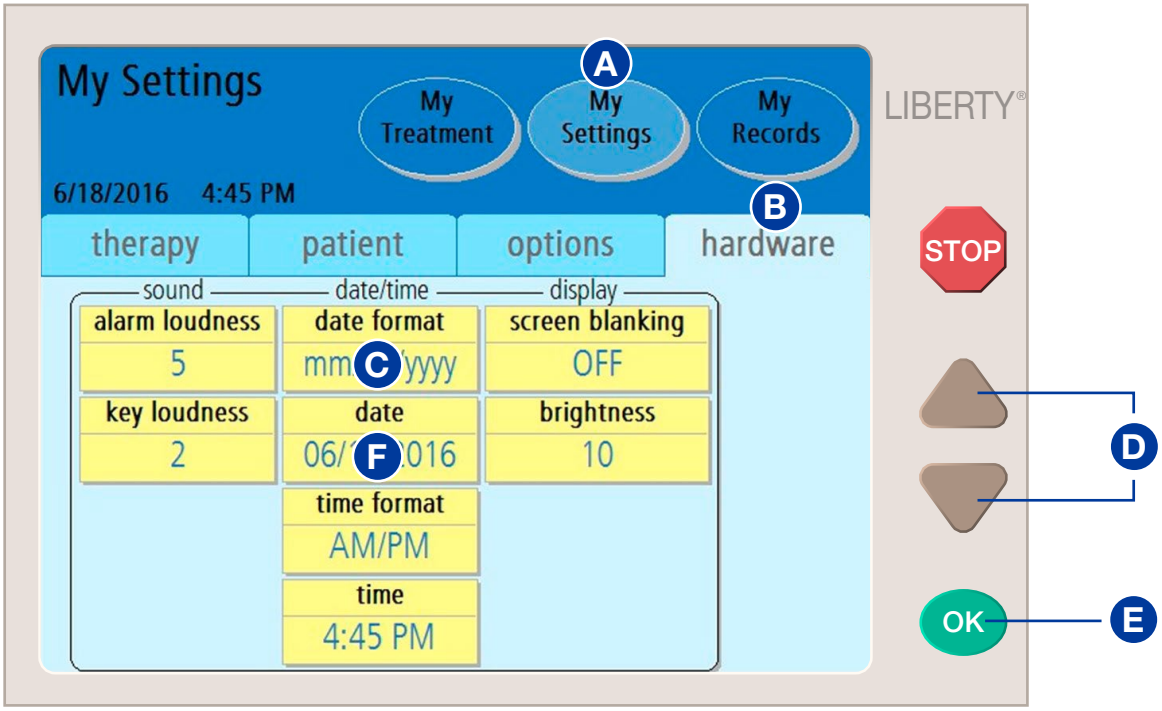

Changing the date

1.	Select **My Settings**	A	
2.	Select **hardware** tab	B	
3.	Select **date format** (Button turns orange)	C	
4.	Use the arrow keys to select **mm/dd/yyyy**	D	
5.	Select **OK** to save (Button turns yellow)	E	
6.	Select **date** (Button turns orange)	F	
7.	Use the arrow keys to select the **month**	D	
8.	Select **OK** to save and proceed to *day*	E	
9.	Use the arrow keys to select the **day**	D	
10.	Select **OK** to save and proceed to *year*	E	
11.	Use the arrow keys to select the **year**	D	
12.	Select **OK** to save (Button turns yellow)	E	

Read the Instructions for Use for safe and proper use of this device. For a complete description of hazards, contraindications, side effects, and precautions, see full package labeling at www.fmcna.com

Indications for Use: The Fresenius Liberty Select Cycler is indicated for acute and chronic peritoneal dialysis.

Caution: Federal (US) law restricts this device to sale by or on the order of a physician.

© 2024 Fresenius Medical Care. All Rights Reserved. Fresenius Medical Care, the triangle logo, and Liberty are trademarks of Fresenius Medical Care Holdings, Inc. or its affiliated companies. All other trademarks are the property of their respective owners. P/N 105759-01 Rev A 09/2024