FRESENIUS MEDICAL CARE

Peritoneal Dialysis

Liberty® Select Cycler Upload to Clinic Troubleshooting Guide

This guide assists in resolving issues that may prevent patient data uploads from the Liberty Select Cycler to the clinic via a **Cellular Gateway**, prior to contacting Technical Support.

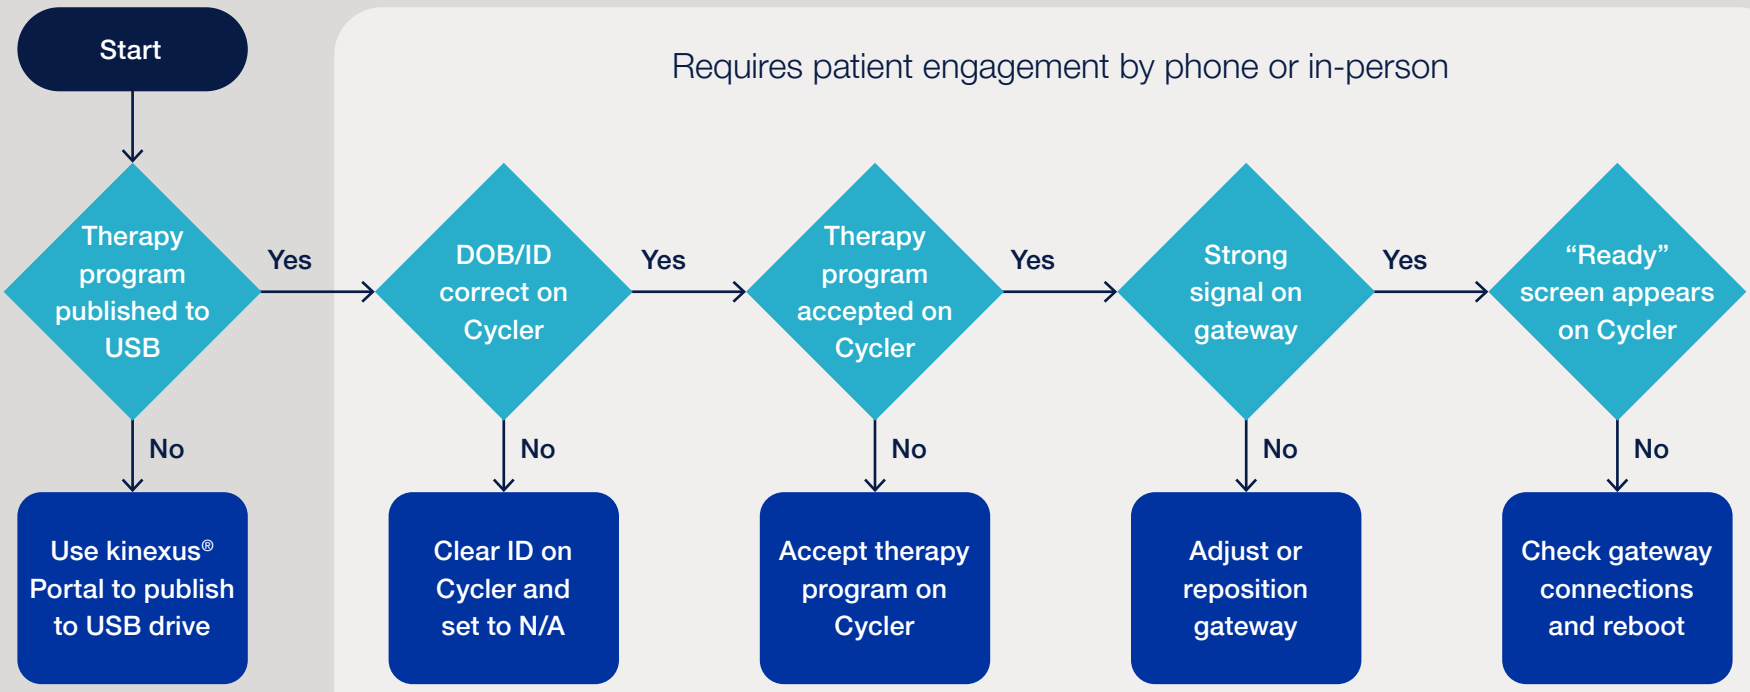

In kinexus portal, publish patient therapy program to a new USB drive

Provide new USB drive to patient with instructions to **Accept** new therapy program on Cycler

Instruct patient to power OFF the Cycler, remove USB drive, then power ON the Cycler

- Press **OK** to clear *No IQdrive detected*
- Select **My Settings** Select **Patient tab** Select **Your ID**. Include correct DOB, if needed
- Delete existing characters and press **Save**
- Press **OK** to accept default setting of *N/A*
- Insert USB drive

Instruct patient to insert USB drive into the Cycler and press **Accept** if therapy was changed

If therapy was not changed, "Ready" screen should appear

Instruct patient to try the following:

- Adjust Gateway antennas for strongest signal while observing Cell strength LEDs
- Relocate the Gateway near a window
- Contact Technical Support

Instruct patient to power OFF the Cycler and try the following:

- Unplug Gateway power for 30 seconds, then plug back in. Wait for Status LED to turn green
- Ensure the cable connected to the Cycler is fully inserted and thumb screws are finger tight
- Unplug Gateway USB cable for 10 seconds, then plug back in
- Power ON Cycler

If issue persists, instruct patient to call Technical Support for further assistance at 1-800-227-2572 (available 24/7)

Read the Instructions for Use for safe and proper use of this device. For a complete description of hazards, contraindications, side effects, and precautions, see full package labeling at www.fmcna.com

Indications for Use: The Fresenius Liberty Select Cycler is indicated for acute and chronic peritoneal dialysis.

Caution: Federal (US) law restricts this device to sale by or on the order of a physician.

Use: The kinexus Gateway is intended for transmission of home dialysis therapy data and patient data for patients using certain Fresenius Medical Care products, including peritoneal dialysis cycler(s).

kinexus is not an electronic health record (EHR) or billing solution.

© 2024 Fresenius Medical Care. All Rights Reserved. Fresenius Medical Care, the triangle logo, Liberty, IQdrive, and kinexus are trademarks of Fresenius Medical Care Holdings, Inc. or its affiliated companies. All other trademarks are the property of their respective owners. P/N 105607-01 RevB 10/2024