FRESENIUS MEDICAL CARE

Connecting an Alternate CAPD System to a stay•safe® Catheter Extension Set.

This procedure is intended to be used in the case that your physician prescribes an alternate continuous ambulatory peritoneal dialysis (CAPD) solution that has a Luer-Lock connector for your long-dwell exchange. Follow these steps to connect that system to your stay•safe catheter extension set.

Notes:

- The use and training for the alternate CAPD system is out of scope for these instructions. Please refer to the manufacturer's Prescribing Information (PI).
- Ensure adequate training is conducted on the use of the PIN connector not typically used with stay•safe CAPD exchanges.
- Follow your center protocols throughout this procedure.
- Do not heat PD solution in a microwave.

Use aseptic technique throughout the procedure.

Prepare

1. Gather supplies. Check expiration dates:
   - stay•safe Luer-Lock Adapter, 4" (P/N 050-95003)
   - Alternate CAPD system and PI
   - Multiple Tubing Segment Set (P/N 050-50758) or stay•safe Drain Set (P/N 026-20030)
   - stay•safe Cap (P/N 050-95012)
2. Face mask as required by center procedure.
3. Prepare your work area and supplies.
4. Mask, wash, and dry hands as taught by your PD nurse.
5. Prepare the stay•safe catheter extension set per center procedure.
6. Prepare the alternate CAPD system per the manufacturer's Prescribing Information (PI).
7. Make sure the white clamp on the catheter extension set is closed.

Connect

1. Unscrew and remove the white sterility cap from square end of the 4” adapter.

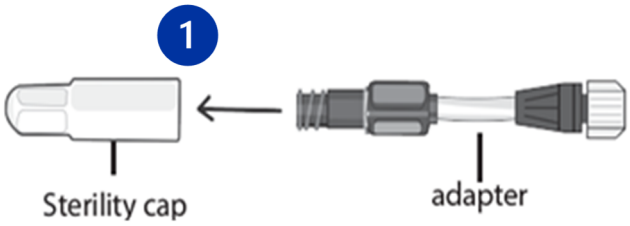

2. Remove the stay·safe cap from the catheter extension set.

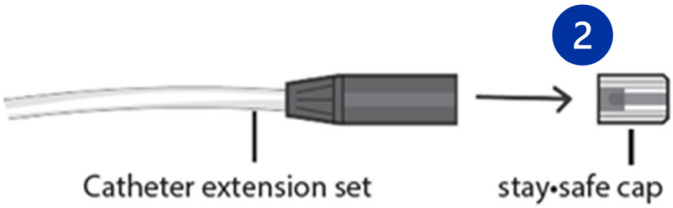

3. Immediately connect square end of 4” adapter to the catheter extension set.

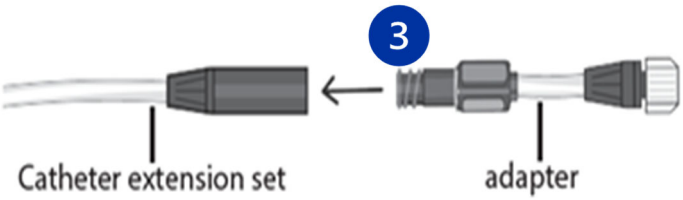

4. Pull the ring off the end of the alternate CAPD system bag line.

5. Remove the white protective cap from the end of 4” adapter and immediately connect it to the Luer-Lock connector on the alternate CAPD system.

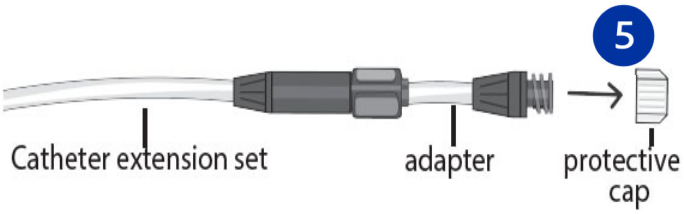

6. Open the white clamp on your catheter extension set and follow the next steps in your CAPD exchange as instructed by your PD nurse.



Disconnect

When the fill is complete, put your mask back on and clean your hands.

Use aseptic technique throughout the procedure.

Use either a Multiple Tubing Segment (MTS) Set or a stay·safe Drain Set to insert a PIN into the end of the catheter extension set as directed by your PD nurse.

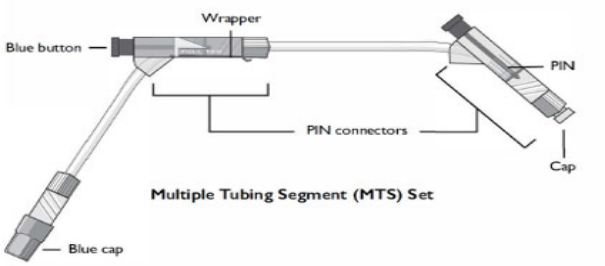



1. Insert the blue clip into the stay·safe Organizer.

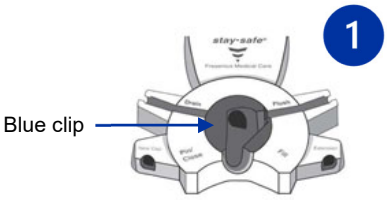

2. Place the PIN connector into the Organizer clip. If using an MTS Set, insert the PIN connector located at the end of the tubing.



3. Place a new stay·safe cap into the left notch of the Organizer.

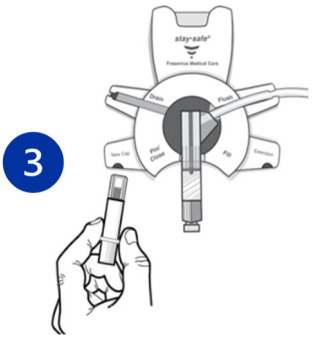

4. Close the white clamp on the catheter extension set.



5. Unscrew the cap from the PIN connector.



6. Disconnect the adapter with the attached alternate CAPD system from the catheter extension set.

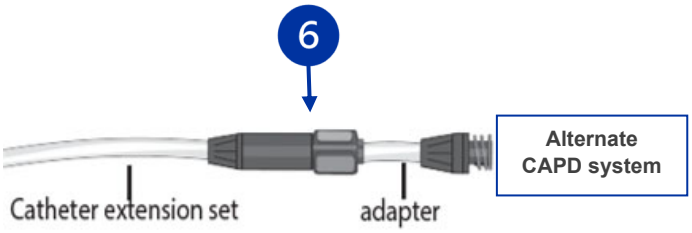

7. Immediately connect the catheter extension set to the PIN connector and open the white clamp on the catheter extension set.

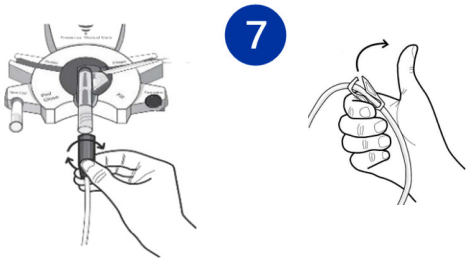

8. Remove PIN connector from the Organizer. Turn the blue button on the PIN connector ¼ turn clockwise to unlock it, then press the blue button to insert the PIN into the catheter extension set.

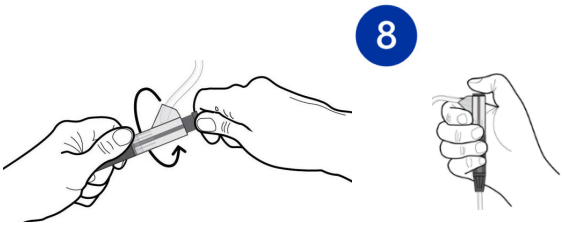

9. Close the white clamp on the catheter extension set.



10. Insert the PIN Connector back into the Organizer clip.



11. Unscrew and remove protective cover from new stay•safe cap and set aside.



12. Unscrew the catheter extension set from the PIN Connector and immediately connect to the new, stay·safe cap.

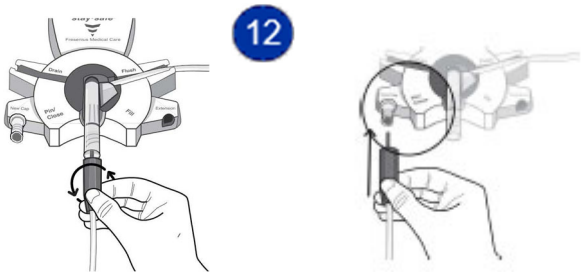

13. Remove catheter extension set from the Organizer. Make sure the cap is tight.

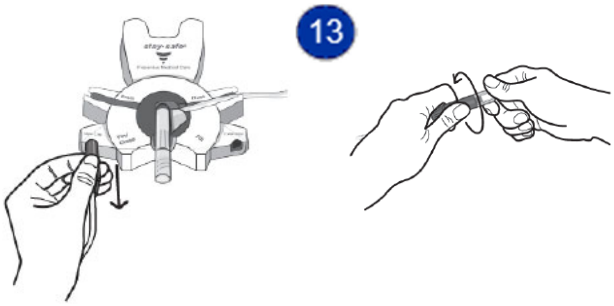

14. Follow your center's procedures for disposal of used items.

Read the Instructions for Use for safe and proper use of these devices. For a complete description of hazards, contraindications, side effects, and precautions, see full package labeling at fmcna.com.

Indications for Use:

The stay·safe catheter extension set with Luer-Lock is indicated for use in patients with acute and chronic end stage renal disease undergoing peritoneal dialysis (PD) in a healthcare facility or at home. The stay·safe catheter extension set with Luer-Lock is used to connect a PD catheter with a Luer-Lock catheter adapter to PD systems that use stay·safe PIN technology.

The stay·safe to Luer-Lock adapter is indicated for use in patients with acute and chronic end-stage renal disease undergoing peritoneal dialysis (PD) in a healthcare facility or at home. The stay·safe to Luer-Lock adapter is used to connect a stay·safe catheter extension set to medical devices with a Luer-Lock connection.

The Multiple Tubing Segment (MTS) Set with stay•safe PIN Connectors is indicated for use by patients with acute and chronic end-stage renal disease undergoing peritoneal dialysis (PD) in a healthcare facility or at home.

The MTS Set is placed during set-up to make additional connections to the cycler set when prescribed or when an interruption in treatment is necessary. This device is compatible with stay•safe Peritoneal Dialysis (PD) connectology system and is to be used only with Fresenius Medical Care (FMCNA) Cyclers and Cycler Sets.

The stay•safe Drain Set is indicated for use by patients with acute and chronic end-stage renal disease undergoing peritoneal dialysis (PD) in a healthcare facility or at home. The stay•safe Drain Set is used to connect directly to the stay•safe catheter extension set to enable drainage and/or effluent sampling as needed.

The Fresenius sterile stay•safe® Cap is intended to be used for closure of the stay•safe peritoneal dialysis connectology system.

Caution: Federal (U.S.) law restricts this device to sale by or on the order of a physician.

© 2023 Fresenius Medical Care. All Rights Reserved. Fresenius Medical Care, the triangle logo, and stay·safe are trademarks of Fresenius Medical Care Holdings, Inc., or its affiliated companies. All other trademarks are the property of their respective owners. P/N 105586-01 Rev A 06/2023